

RNA Clean-Up and Concentration 96-Well Kit

Product # 25100

Product Insert

Norgen's RNA Clean-Up and Concentration 96-Well Kit provides a rapid method for the purification, cleanup and concentration of up to 50 µg of RNA isolated using different methods including phenol/guanidine-based protocols, and from various upstream enzymatic reactions such as DNase treatment and labeling. This kit can also be used for the clean-up and concentration of RNA transcripts from *in vitro* transcription reactions by removing polymerases, unincorporated dNTPs, salts and DTT (please see Appendix B). The kit purifies all sizes of RNA, from large mRNA and ribosomal RNA down to microRNA (miRNA) and small interfering RNA (siRNA). The RNA is preferentially purified from other reaction components such as proteins, RNases and nucleotides, without the use of phenol or chloroform. The purified RNA is of the highest integrity, and can be used in a number of downstream applications including end-point or quantitative reverse transcription PCR, Northern blotting, RNase protection and primer extension, and expression array assays.

Norgen's Purification Technology

Purification is based on 96-well column chromatography using Norgen's proprietary resin as the separation matrix. The RNA, including RNA transcripts, is preferentially purified from impurities such as proteins, salts, polymerases and nucleotides without the use of phenol or chloroform. The process involves first mixing the RNA samples, the *in vitro* transcription reaction sample, or the enzymatic reaction containing RNA with Buffer RL (please see the flow chart on page 4). The appropriate alcohol is then added and the mixture is loaded onto a 96-Well Plate. Norgen's resin binds RNA in a manner that depends on ionic concentrations. Thus only the RNA will bind to the resin in the wells, while the contaminating proteins or nucleotides will be removed in the flowthrough. The bound RNA is then washed three times with the provided Wash Solution A in order to remove any remaining impurities, and the purified RNA is eluted with the Elution Solution A. The purified RNA is of the highest integrity, and can be used in a number of downstream applications. Norgen's RNA Clean-Up and Concentration 96-Well Kit purifies RNA with minimal amounts of DNA contamination. An optional protocol is provided in Appendix A for maximum removal of residual DNA that may affect sensitive downstream applications such as quantitative PCR.

Specifications

Kit Specifications	
Binding Capacity per Well	50 µg
Size of RNA Purified	All sizes, including small RNA (<200 nt)
Maximum Amount of Starting Material:	50 µg of RNA
Minimum Elution Volume	75 µL
Time to Complete 10 Purifications	30 minutes
Average Recovery	≥ 90%

Advantages

- Efficient RNA cleanup from various enzymatic reactions – labeling, DNase treatment and *in vitro* transcription
- Cleanup of RNA isolated using different methods, including phenol/chloroform extractions
- Fast and easy processing using either a vacuum manifold or centrifugation
- Suitable for all sizes of RNA, from large rRNA down to microRNA (miRNA)
- No phenol or chloroform extractions

Kit Components

Component	Product # 25100 (192 preps)
Buffer RL	2 x 40 mL
Wash Solution A	2 x 38 mL
Elution Solution A	2 x 20 mL
96-Well Plate	2
Adhesive Tape	4
96-Well Collection Plate	2
96-Well Elution Plate	2
Product Insert	1

Storage Conditions and Product Stability

All solutions should be kept tightly sealed and stored at room temperature. These reagents should remain stable for at least 2 years in their unopened containers.

Precautions and Disclaimers

This kit is designed for research purposes only. It is not intended for human or diagnostic use. Ensure that a suitable lab coat, disposable gloves and protective goggles are worn when working with chemicals. For more information, please consult the appropriate Material Safety Data Sheets (MSDSs). These are available as convenient PDF files online at www.norgenbiotek.com.

The Buffer RL contains guanidinium salts, and should be handled with care. Guanidinium salts form highly reactive compounds when combined with bleach, thus care must be taken to properly dispose of any of these solutions

Customer-Supplied Reagents and Equipment

For All Protocols

- For **Vacuum Format**:
 - Vacuum manifold with vacuum pump capable of generating a minimum pressure of -650 mbar or -25 in. Hg (such as Whatman UniVac 3 Vacuum to Collect Manifold)
 - Sealing tape or pads
- For **Centrifuge Format**:
 - Centrifuge with rotor for 96-well plate assembly (such as Thermo Fisher IEC Centra CL3 series or Beckman GS-15R)

For RNA Clean-Up and Concentration from Enzymatic Reactions or Non-Phenol/Guanidine-Based RNA Isolation Methods

- β -mercaptoethanol
- 96 - 100% ethanol
- RNase-free or DEPC-treated water

For RNA Clean-Up and Concentration from Phenol/Guanidine-Based RNA (Trizol or Tri Reagent) Isolation Methods

- 70% ethanol

For RNA Clean-Up and Concentration from in vitro transcription reactions

- β -mercaptoethanol
- Isopropanol

Working with RNA


RNases are very stable and robust enzymes that degrade RNA. Autoclaving solutions and glassware is not always sufficient to actively remove these enzymes. The first step when preparing to work with RNA is to create an RNase-free environment. The following precautions are recommended as your best defense against these enzymes.

- The RNA area should be located away from microbiological work stations
- Clean, disposable gloves should be worn at all times when handling reagents, samples, pipettes, disposable tubes, etc. It is recommended that gloves are changed frequently to avoid contamination
- There should be designated solutions, tips, tubes, lab coats, pipettes, etc. for RNA only
- All RNA solutions should be prepared using at least 0.05% DEPC-treated autoclaved water or molecular biology grade nuclease-free water
- Clean all surfaces with commercially available RNase decontamination solutions
- When working with purified RNA samples, ensure that they remain on ice during downstream applications

Flow Chart

Procedure for Purifying RNA using Norgen's RNA Clean-up and Concentration 96-Well Kit

RNA Clean-Up and Concentration 96-Well Kit Procedure

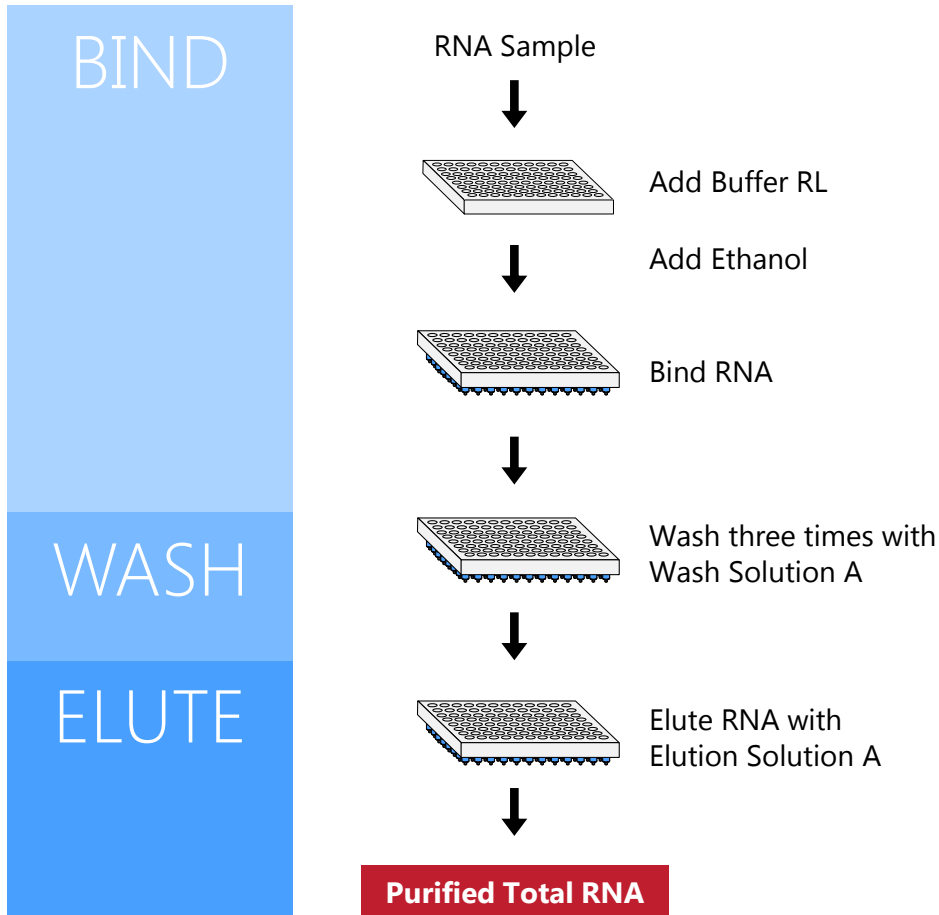

Procedures

For Vacuum Manifold: All vacuum steps are performed at room temperature. The correct pressure can be calculated using the conversions:

$$1 \text{ mbar} = 100 \text{ Pa} = 0.0394 \text{ in. Hg} = 0.75 \text{ mm Hg} = 0.0145 \text{ psi}$$

For Centrifugation: All centrifugation steps are performed at room temperature. The correct rpm can be calculated using the formula:

$$\text{RPM} = \sqrt{\frac{\text{RCF}}{(1.118 \times 10^{-5}) (r)}}$$

where *RCF* = required gravitational acceleration (relative centrifugal force in units of g); *r* = radius of the rotor in cm; and *RPM* = the number of revolutions per minute required to achieve the necessary *g*-force.

Notes Prior to Use

- **The steps for sample preparation are different depending on your starting material.**
 - For sample preparation for RNA clean-up and concentration from enzymatic reactions or non-phenol/guanidine-based RNA isolation methods please follow **Section 1A**.
 - For sample preparation for RNA clean-up and concentration from phenol/guanidine-Based RNA (Trizol or Tri Reagent) isolation methods please follow **Section 1B**.
 - For sample preparation for RNA transcript Clean-up and Concentration starting from *in vitro* transcription reactions please follow **Section 1C**.
- Once the sample has been prepared RNA clean-up can be performed using either a vacuum manifold or centrifugation. For purification using vacuum, please follow the procedure outlined in **Section 2A**. For purification using centrifugation, please follow the procedure outlined in **Section 2B**.
- Ensure that all solutions are at room temperature prior to use.
- Prepare a working concentration of the **Wash Solution A** by adding 90 mL of 96 - 100% ethanol (provided by the user) to the supplied bottles containing the concentrated **Wash Solution A**. This will give a final volume of 128 mL. The label on the bottles has a box that may be checked to indicate that the ethanol has been added.
- It is recommended that no more than 50 µg of RNA to be used per cleanup.
- The volumes stated in each procedure for input preparation are the volumes required to prepare samples for each well of the 96-well plate.
- It is important to work quickly during this procedure.
- This kit purifies RNA with minimal amounts of DNA contamination. However, an optional protocol is provided in Appendix A for maximum removal of residual DNA that may affect sensitive downstream applications such as quantitative PCR. The procedure in Appendix A is to be carried out prior to performing the kit procedure below.

Section 1. Sample Preparation

A. Sample Preparation for RNA Clean-Up and Concentration from Enzymatic Reactions or Non-Phenol/Guanidine-Based RNA Isolation Methods

Notes Prior to Use

- Prepare an appropriate amount of Buffer RL by adding 10 µL of β-mercaptoethanol (provided by the user) to each 1 mL of Buffer RL required. β-mercaptoethanol is toxic and should be dispensed in a fume hood.

1. Sample Preparation

- a. Adjust the volume of the RNA sample to 100 µL by adding RNase-free or DEPC-treated water. It is recommended that no more than 50 µg of RNA be used for each well.
- b. Add 200 µL of **Buffer RL** to the RNA sample. Mix by vortexing
- c. Add 120 µL of 96 – 100% ethanol (provided by the user) to the mixture from step **1b**. Mix by vortexing for 10 seconds.
- d. RNA purification can now be performed using either a vacuum manifold or centrifugation. For purification using vacuum, please follow the procedure outlined in Section 2A. For purification using centrifugation, please follow the procedure outlined in Section 2B.

B. Sample Preparation for RNA Clean-up and Concentration from Phenol/Guanidine-Based RNA (Trizol or Tri Reagent) Isolation Methods

Notes Prior to Use

- The loading capacity of each well in the 96-Well Plate is 500 μL . Depending on the aqueous phase volume after the phase separation, the subsequent binding step may need to be repeated once or more. For example, if the aqueous phase volume is 500 μL , an additional 500 μL of 70% EtOH will be added for a final volume of 1 mL. The binding will be repeated once in order to have all input passed through the column.

1. Sample Preparation

- a. Isolate RNA using a phenol/guanidine-based reagent such as Trizol or Tri Reagent, according to manufacturer's instruction. After the separation of the aqueous and organic phases, collect the upper (aqueous) fraction containing the RNA into a new RNase-free microcentrifuge tube (not provided). Note the volume.
- b. Add one volume of 70% ethanol (provided by the user) to the fraction from step **1a**. Mix by vortexing for 10 seconds.
- c. RNA purification can now be performed using either a vacuum manifold or centrifugation. For purification using vacuum, please follow the procedure outlined in Section 2A. For purification using centrifugation, please follow the procedure outlined in Section 2B.

C. Sample Preparation for RNA Transcript Clean-up and Concentration from *in vitro* Transcription Reactions

Notes Prior to Use

- Prepare an appropriate amount of **Buffer RL** by adding 10 μL of β -mercaptoethanol (provided by the user) to each 1 mL of Buffer RL required. β -mercaptoethanol is toxic and should be dispensed in a fume hood.
- Digestion of the DNA template used in the *in vitro* transcription reaction should be performed before cleaning the RNA transcript. Ensure that RNase-free DNase is used for the digestion step.
- The procedure below outlines the sample preparation of 100 μL and 200 μL of *in vitro* transcription reaction. The volumes of solutions to be used for 100 μL are stated first, and the volumes of solutions for be used for 200 μL are shown in brackets

1. Sample Preparation

- a. Adjust the volume of the RNA sample to 100 μL (200 μL) by adding RNase-free or DEPC-treated water. It is recommended that no more than 50 μg of RNA be used for each well.
- b. Add 250 μL (500 μL) of **Buffer RL** to the RNA sample. Mix by vortexing
- c. Add 250 μL (500 μL) of isopropanol (provided by the user) to the mixture from step **1b**. Mix by vortexing for 10 seconds.
- d. RNA purification can now be performed using either a vacuum manifold or centrifugation. For purification using vacuum, please follow the procedure outlined in Section 2A. For purification using centrifugation, please follow the procedure outlined in Section 2B.

Section 2. RNA Clean-Up and Concentration from All Types of Input

Note: The purification of RNA mix prepared in Section 1 could be performed using either a vacuum manifold or centrifugation. For purification using vacuum, please follow the procedure outlined in Section 2A. For purification using centrifugation, please follow the procedure outlined in Section 2B

A. Clean-Up and Concentration Using Vacuum Manifold

1. Binding RNA to 96-Well Plate

- a. Assemble the 96-Well Plate and the vacuum manifold according to manufacturer's recommendations.

Note: The provided 96-Well Collection Plate can be used as the collection/waste tray if desired.

- b. Apply up to 500 μL of the input with the ethanol (from **Section 1**) into each well of the 96-Well Plate. Tape the plate or any unused wells using sealing tape or pads (provided by the user) according to the vacuum manifold manufacturer's recommendations. Apply vacuum for 2 minutes.

Note: Depending on the starting material, a small quantity of precipitates may appear in the input-ethanol mix. No additional step is required to remove these precipitates prior to application of the mixture to the wells.

- c. Turn off vacuum and ventilate the manifold. Discard the flowthrough. Reassemble the 96-Well Plate and the vacuum manifold.

Note: Ensure that all of the input from each well has passed through into the collection/waste tray. If the entire input volume has not passed, apply vacuum for an additional 2 minutes.

- d. If the input RNA mix volume is greater than 500 μL , repeat Step **1a** to Step **1c** until all the input has passed through the 96-Well Plate.

2. RNA Wash

- a. Apply 400 μL of **Wash Solution A** to each well of the 96-Well Plate. Tape the plate or any unused wells using sealing tape or pads (provided by the user) according to the vacuum manifold manufacturer's recommendations. Apply vacuum for 2 minutes.

Note: Ensure the entire Wash Solution A has passed through into the collection/waste tray by inspecting the 96-Well Plate. If the entire wash volume has not passed, apply vacuum for an additional 2 minutes.

- b. Turn off vacuum and ventilate the manifold. Discard the flowthrough.
- c. Reassemble the 96-Well Plate and the vacuum manifold. Repeat steps **2a** and **2b** to wash column for a second time.
- d. Reassemble the 96-Well Plate and the vacuum manifold. Repeat steps **2a** and **2b** to wash column for a third time.
- e. Pat the bottom of the 96-Well Plate dry. Reassemble the 96-Well Plate and the vacuum manifold. Apply vacuum for an additional 5 minutes in order to completely dry the plate.
- f. Turn off vacuum and ventilate the manifold.

4. RNA Elution

- a. Remove the lid from the provided Elution Plate. Replace the collection/waste tray in the vacuum manifold with the Elution Plate. Complete the vacuum manifold assembly with the 96-Well Plate.
- b. Add 75 μL of **Elution Solution A** to each well of the plate.
- c. Apply vacuum for 2 minutes.

5. Storage of RNA

Use the provided adhesive tape and/or lid to seal the Elution Plate. The purified RNA samples may be stored at -20°C for a few days. It is recommended that samples be placed at -70°C for long term storage.

B. Clean-Up and Concentration Using Centrifugation

1. Binding RNA to 96-Well Plate

- a. Place the 96-Well Plate on top of a provided 96-Well Collection Plate.
- b. Apply up to 500 μL of the input with the ethanol (from **Section 1**) into each well of the 96-Well Plate. Centrifuge the assembly at maximum speed or $3,000 \times g$ ($\sim 3,000$ RPM) for 2 minutes.

Note: Depending on the starting material, a small quantity of precipitates may appear in the input-ethanol mix. No additional step is required to remove these precipitates prior to application to the wells

- c. Discard the flowthrough. Reassemble the the 96-Well Plate and the bottom plate.

Note: Ensure that all of the input from each well has passed through into the bottom plate. If the entire input volume has not passed, centrifuge for an additional 2 minutes.

- d. If the input RNA mix volume is greater than 500 μL , repeat Step **1a** to Step **1c** until all the input has passed through the 96-Well Plate.

2. RNA Wash

- a. Apply 400 μL of **Wash Solution A** to each well of the 96-Well Plate. Centrifuge the assembly at maximum speed or $3,000 \times g$ ($\sim 3,000$ RPM) for 2 minutes.

Note: Ensure the entire Wash Solution A has passed through into the bottom plate by inspecting the 96-Well Plate. If the entire wash volume has not passed, centrifuge for an additional 2 minutes.

- b. Discard the flowthrough. Reassemble the 96-Well Plate and the bottom plate.
- c. Repeat steps **2a** and **2b** to wash column for a second time.
- d. Repeat steps **2a** and **2b** to wash column for a third time.
- e. Pat the bottom of the 96-Well Plate dry. Reassemble the 96-Well Plate and the bottom plate. Centrifuge the assembly at maximum speed or $3,000 \times g$ ($\sim 3,000$ RPM) for 5 minutes in order to completely dry the plate.

3. RNA Elution

- a. Remove the lid from the provided Elution Plate. Stack the 96-Well Plate on top of the Elution Plate.
- b. Add 75 μL of **Elution Solution A** to each well of the 96-Well Plate.
- c. Centrifuge the assembly at maximum speed or $3,000 \times g$ ($\sim 3,000$ RPM) for 2 minutes.

4. Storage of RNA

Use the provided adhesive tape and/or lid to seal the Elution Plate. The purified RNA sample may be stored at -20°C for a few days. It is recommended that samples be placed at -70°C for long term storage.

Appendix A

Protocol for Optional On-Column DNA Removal

Norgen's RNA Clean-Up and Concentration 96-Well Kit isolates total RNA with minimal amounts of genomic DNA contamination. However, an optional protocol is provided below for maximum removal of residual DNA that may affect sensitive downstream applications. It is recommended that Norgen's RNase-Free DNase I Kit (Product # 25710) be used for this step.

1. For every on-column reaction to be performed, prepare a mix of 10 μL of **DNase I** and 65 μL of **Enzyme Incubation Buffer** using Norgen's RNase-Free DNase I Kit (Product # 25710). Mix gently by inverting the tube a few times. **DO NOT VORTEX**.

Note: If using an alternative DNase I, prepare a working stock of 0.25 Kunitz unit/ μL RNase-free DNase I solution according to the manufacturer's instructions. A 75 μL aliquot is required for each column to be treated.

2. Perform the appropriate RNA Cleanup Procedure for your starting material up to and including "**Binding RNA to 96-Well Plate**" (Steps 1 and 2 of all protocols)
3. **For Vacuum Manifold:** Apply 400 μL of **Wash Solution A** to each well of the 96-Well Plate. Tape the plate or any unused wells using sealing tape or a pad (provided by the user) according to the vacuum manifold manufacturer's recommendations. Apply vacuum for 2 minutes.

For Centrifugation: Apply 400 μL of **Wash Solution A** to each well of the 96-Well Plate. Centrifuge the assembly at maximum speed or 3,000 $\times g$ (~3,000 RPM) for 2 minutes.

4. Discard the flowthrough. Reassemble the 96-Well Plate with the vacuum manifold or the bottom plate.
5. Apply 75 μL of the RNase-free DNase I solution prepared in Step 1 to each well of the 96-Well Plate.

For Vacuum Manifold: Apply vacuum for 30 seconds.

For Centrifugation: Centrifuge the assembly at maximum speed or 3,000 $\times g$ (~3,000 RPM) for 30 seconds.

6. After the centrifugation or vacuum in Step 5, pipette the flowthrough that is present in the collection plate back onto the top of the column.

Note: Ensure Step 6 is performed in order to ensure maximum DNase activity and to obtain maximum yields of RNA, in particular for small RNA species

7. Incubate the assembly at 25 - 30°C for 15 minutes.
8. Without any further centrifugation, proceed directly to "**RNA Wash**" Section 2A, Step 3b for **Vacuum Manifold** procedure or Section 2B, Step 3c for **Centrifugation** procedure.

Troubleshooting Guide

Problem	Possible Cause	Solution and Explanation
Poor RNA Recovery	Wells of the plate have become clogged	Do not exceed the recommended amounts of starting materials. The amount of starting material may need to be decreased if the wells of the plate show clogging below the recommended levels. See also “Clogged Wells in Plate” below.
	An alternative elution solution was used	It is recommended that the Elution Solution A supplied with this kit be used for maximum RNA recovery.
	Ethanol was not added to the input	Ensure that the appropriate amount of ethanol is added to the input before binding to the column.
	Ethanol was not added to the Wash Solution A	Ensure that 90 mL of 96 - 100% ethanol is added to the supplied Wash Solution A prior to use.
Clogged Wells in Plate	High amounts of RNA in the input	Ensure that no more than 50 µg of RNA is used as the input for each well of the plate.
	High amounts of genomic DNA present in sample	The input may be passed through a 25 gauge needle attached to a syringe 5-10 times in order to shear the genomic DNA prior to loading onto the column.
	Centrifuge temperature too low	Ensure that the centrifuge remains at room temperature throughout the procedure. Temperatures below 15°C may cause precipitates to form that can cause the wells to clog.
	Insufficient Vacuum	Ensure that a vacuum pressure of at least -650 mbar or -25 in. Hg is developed
RNA is Degraded	RNase contamination	RNases may be introduced during the use of the kit. Ensure proper procedures are followed when working with RNA. Please refer to “ <i>Working with RNA</i> ” at the beginning of this user guide.
	Procedure not performed quickly enough	In order to maintain the integrity of the RNA, it is important that the procedure be performed quickly.
	Improper storage of the purified RNA	For short term storage RNA samples may be stored at -20°C for a few days. It is recommended that samples be stored at -70°C for longer term storage.

Problem	Possible Cause	Solution and Explanation
RNA does not perform well in downstream applications	RNA was not washed three times with the provided Wash Solution A	Traces of salt from the binding step may remain in the sample if the column is not washed three times with the Wash Solution A. Salt may interfere with downstream applications, and thus must be washed from the column.
	Ethanol carryover	Ensure that the dry spin under the Column Wash procedure is performed, in order to remove traces of ethanol prior to elution. Ethanol is known to interfere with many downstream applications.
DNA or Genomic DNA contamination	Large amounts of starting material used	Perform RNase-free DNaseI digestion on the RNA sample prior to starting the protocol as outlined in Appendix A.

Related Products	Product #
Total RNA Purification Kit	17200
Cytoplasmic & Nuclear RNA Purification Kit	21000
Leukocyte RNA Purification Kit	21200
microRNA Purification Kit	21300
100b RNA Ladder	15002
1kb RNA Ladder	15003

Technical Support

Contact our Technical Support Team between the hours of 8:30 and 5:30 (Eastern Standard Time) at (905) 227-8848 or Toll Free at 1-866-667-4362.

Technical support can also be obtained from our website (www.norgenbiotek.com) or through email at techsupport@norgenbiotek.com.

Norgen's purification technology is patented and/or patent pending. See www.norgenbiotek.com/patents

3430 Schmon Parkway, Thorold, ON Canada L2V 4Y6
Phone: (905) 227-8848
Fax: (905) 227-1061
Toll Free in North America: 1-866-667-4362